

Reference	ESI	Calibration date	June 25 2021
Ref P/N	SR104	Ambient Temperature	22.97 °C
Serial	834026	Relative Humidity	43.97 %
ID Number	Thermistor transfer	Pressure	1022.08 hPa
Notes	Both SR104 isothermal at +23.0 °C	Test type	Datron 1281 nulled DMM ports, TrueOHM, RESL8

Reference standard	Mfg	Model	Options	Serial / Unc	CEID	Calibration date	Due date
10KR STD	ESI	SR104	10000.0388 Ω	834026	C1210609	06/10/2021	06/10/2022
DMM	Datron	1281			XTR2	06/25/2021	06/25/2022

xDevs.com certifies that this calibration used standards whose accuracies are traceable to the SI, through ISO 17025 Accredited Measurement Laboratory. Actual measurement uncertainty available upon request was calculated using the expanded method and is expressed in values at approximately the 95% confidence level using a coverage factor of K= 2.

Certificate statements are based on test results within specified limits without reduction of the uncertainty of the test and/or measurement. The test and measurement data here relate only to the item tested and/or measured. Unit acceptance of failure includes uncertainty data compilation. Calibration due date that appears on the Certificate of Calibration and labels are determined by the customer and does not imply conformance to a standard.



UUT output transferred by manual ratiometric measurement with reference standard.

Fixed 10000 Ω TrueOhm range is used on the Datron 1281 detector. The following test use 10 minute transfer specification with ESI SR104 output source as reference. Gain verified for stability ±0.10 ppm over the test period. Detector zero offset is DUT is nulled prior to the measurement.

Configuration : RESL8, FILT_OFF, XFER, LOI_OFF, Guarded, PTFE wiring on FRONT, CH_A, CH_B ports.

	Measurement	Unit	Uncertainty	Standard Deviation	DUT Spec / Δ	Degree of freedom / Notes
Transfer reference output	10000.0388	Ω	±0.110 ppm			
Reference measured output (+)	10000.0350	Ω	±0.300 ppm	σ = 7.668768e-04 Ω	Δ = -0.380 ppm	15
Reference calculated +/-	10000.0350	Ω	±0.300 ppm		Δ = -0.380 ppm	
Detector zero offset	0.0000	Ω		σ = 1.050057e-07 Ω		
UUT measured output (+)	10002.0480	Ω	±0.300 ppm	σ = 9.615092e-04 Ω		15
Ratio positive polarity	1.00020130		±0.600 ppm			Inf
UUT calculated output (+)	10002.0518	Ω	±0.710 ppm		Δ = 0.000 ppm	
Temperature Δ	-0.332	°C	±0.60 °C		±1.0 °C	
UUT previous data	10001.9117	Ω	±0.100 ppm			Report
Deviation from previous measurement	14.007 ppm	Ω				
UUT Expanded measurement (Linear) k=2	10002.0518	Ω	±0.710 ppm		0.1%	In spec
UUT Expanded measurement (RSS) k=2	10002.0518	Ω	±0.610 ppm		0.1%	In spec

[Statistics image data](#)

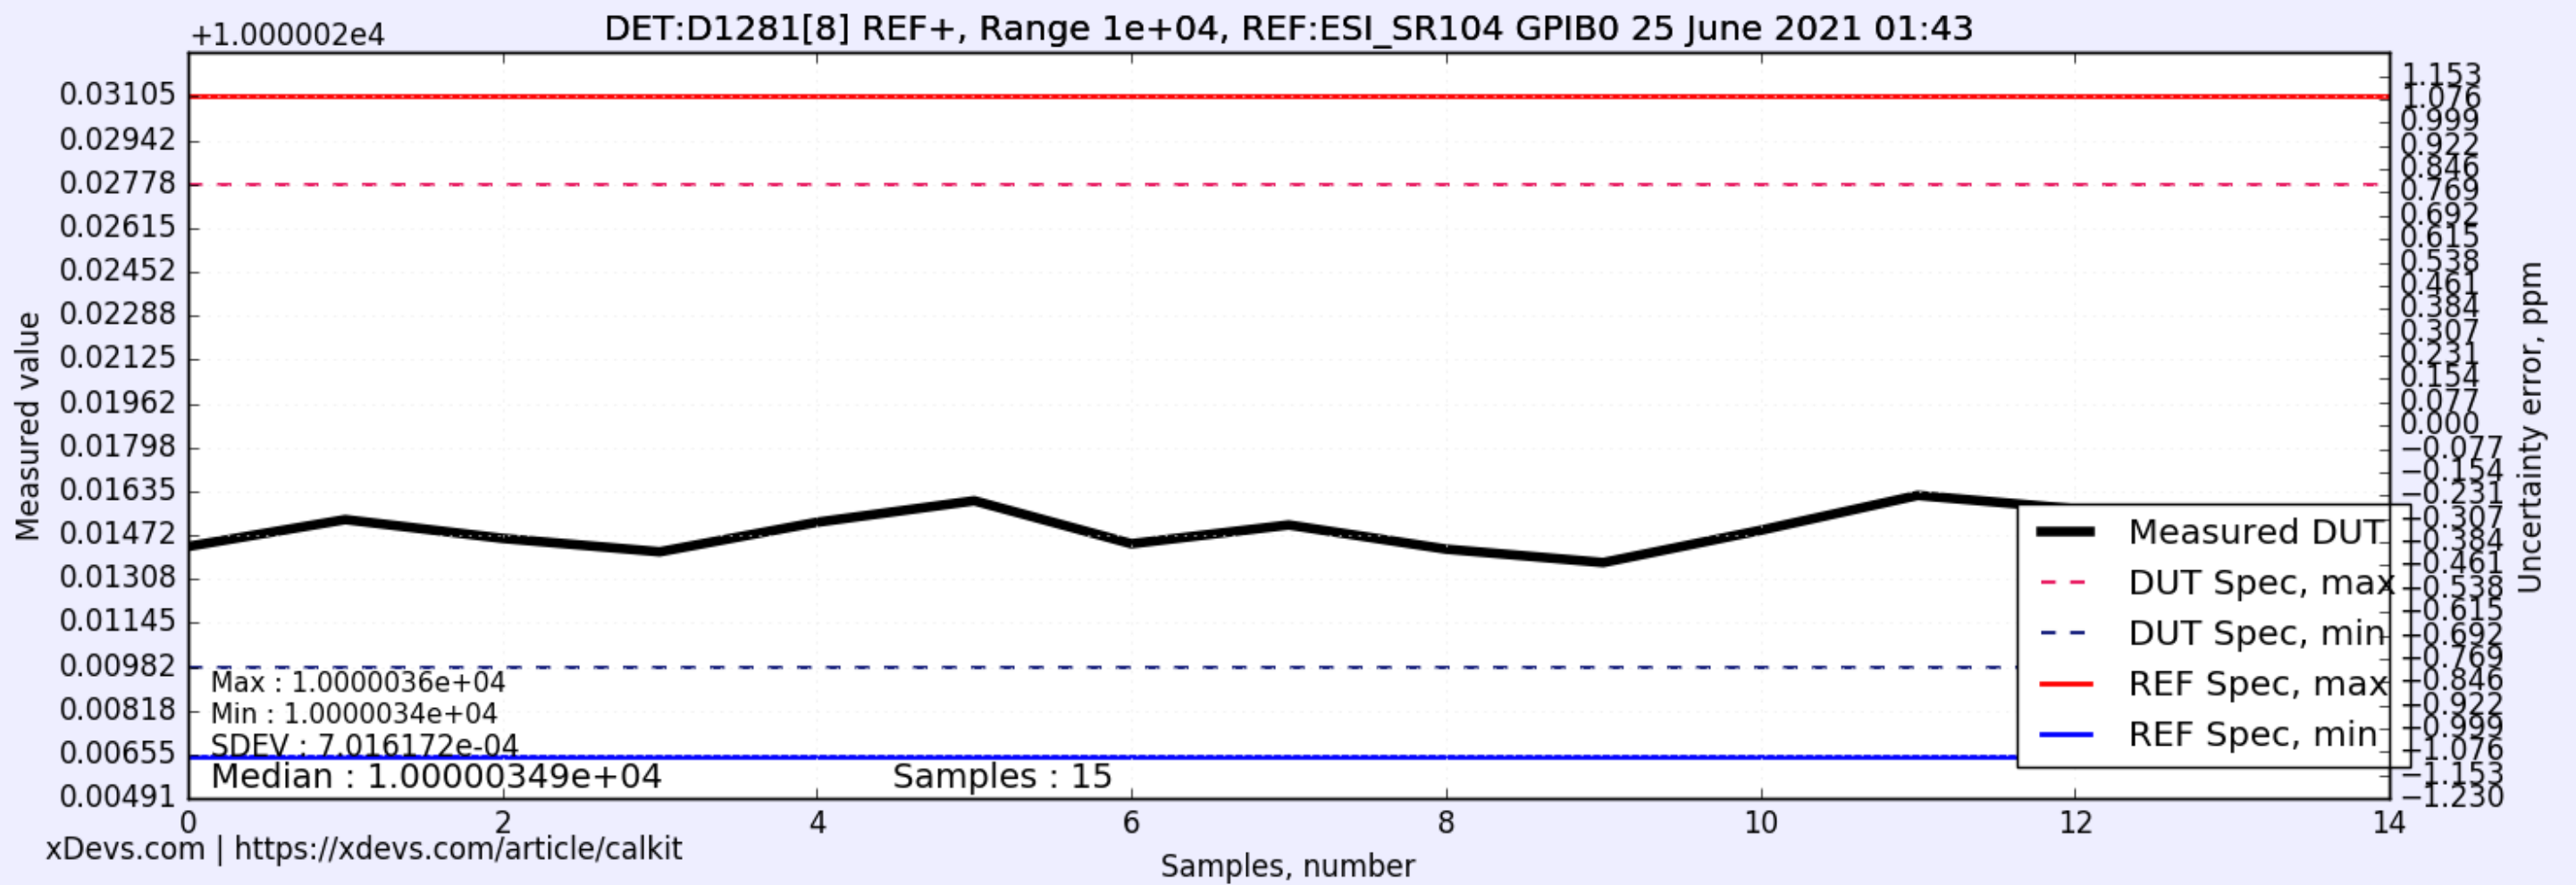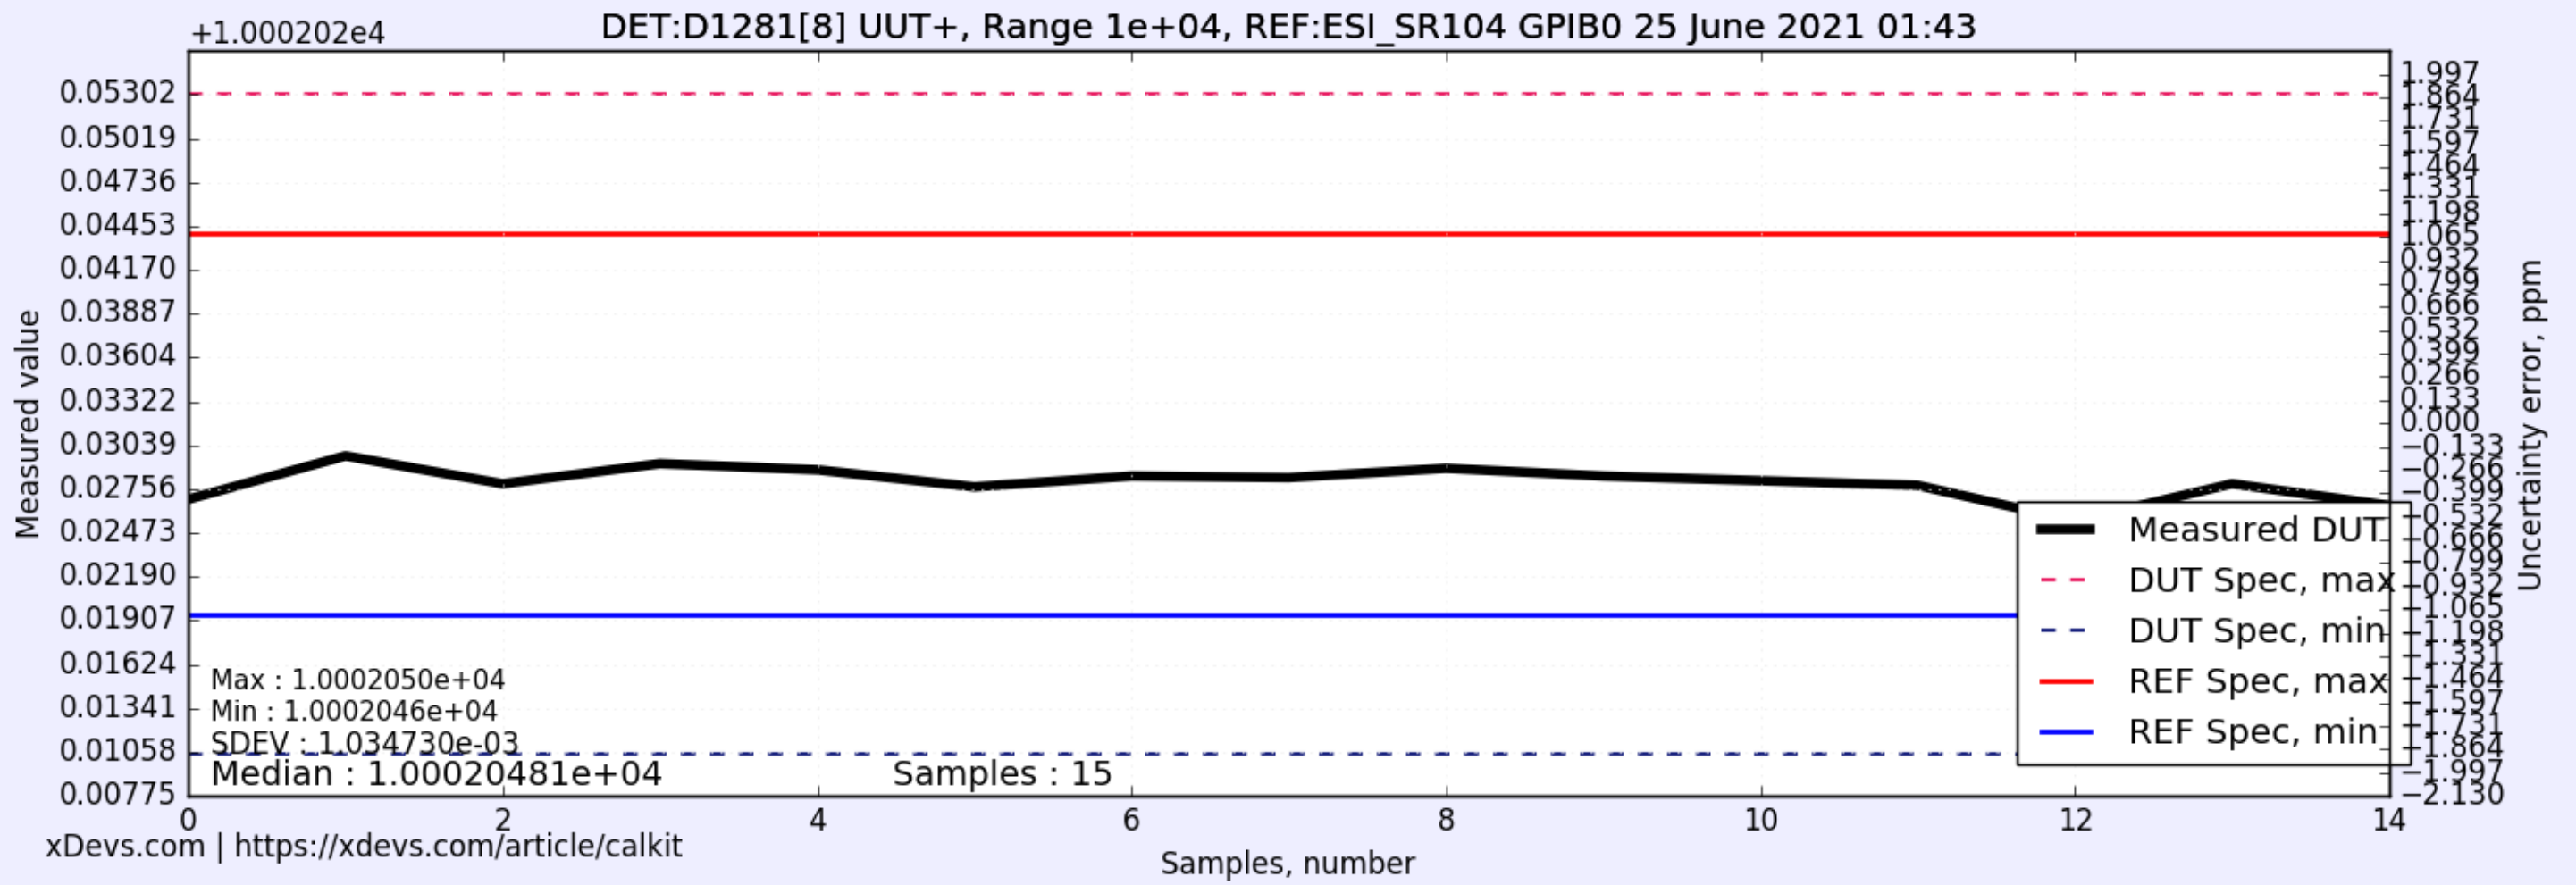

Internal data, do not expose

RAW data	Result
Array Ref P	[10000.0343, 10000.0353, 10000.0346, 10000.0341, 10000.0352, 10000.036, 10000.0344, 10000.0351, 10000.0342, 10000.0337, 10000.0349, 10000.0362, 10000.0357, 10000.0354, 10000.0347]
Array Ref N	∅
Array UUT P	[10002.0469, 10002.0497, 10002.0479, 10002.0492, 10002.0488, 10002.0477, 10002.0484, 10002.0483, 10002.0489, 10002.0484, 10002.0481, 10002.0478, 10002.0455, 10002.0479, 10002.0465]
Array UUT N	∅

Histogramm

