

## Keysight E1779A Battery Pack

This manual provides documentation for the following analyzers:

### Keysight ESA-E Series

E4401B (9 kHz- 1.5 GHz)

E4405B (9 kHz - 13.2 GHz)

E4402B (9 kHz - 3.0 GHz)

E4407B (9 kHz - 26.5 GHz)

E4404B (9 kHz - 6.7 GHz)

### Keysight ESA-L Series

E4411B (9 kHz- 1.5 GHz)

E4403B (9 kHz - 3.0 GHz)

E4408B (9 kHz - 26.5 GHz)

### Keysight EMC Series

E7401A (9 kHz- 1.5 GHz)

E4405B (9 kHz - 13.2 GHz)

E4407B (9 kHz - 26.5 GHz)

E7402A (9 kHz - 3.0 GHz)

E7403A (9 kHz - 6.7 GHz)

Notice: This document contains references to Agilent. Please note that Agilent's Test and Measurement business has become Keysight Technologies. For more information, go to [www.keysight.com](http://www.keysight.com).

## Notices

© Keysight Technologies, Inc.  
2009-2014

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies as governed by United States and international copyright laws.

### Trademark Acknowledgements

### Manual Part Number

E1779-90017

### Print Date

October 2014

Published in USA

Keysight Technologies Inc.  
1400 Fountaingrove Parkway  
Santa Rosa, CA 95403

### Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

### Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

### Restricted Rights Legend

If software is for use in the performance of a U.S. Government prime contract or subcontract, Software is delivered and licensed as

"Commercial computer software" as defined in DFAR 252.227-7014 (June 1995), or as a "commercial item" as defined in FAR 2.101(a) or as "Restricted computer software" as defined in FAR 52.227-19 (June 1987) or any equivalent agency regulation or contract clause. Use, duplication or disclosure of Software is subject to Keysight Technologies' standard commercial license terms, and non-DOD Departments and Agencies of the U.S. Government will receive no greater than Restricted Rights as defined in FAR 52.227-19(c)(1-2) (June 1987). U.S. Government users will receive no greater than Limited Rights as defined in FAR 52.227-14 (June 1987) or DFAR 252.227-7015 (b)(2) (November 1995), as applicable in any technical data.

## Safety Notices

### CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

### WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

## Where to Find the Latest Information

Documentation is updated periodically. For the latest information about these products, including instrument software upgrades, application information, and product information, browse to one of the following URLs, according to the name of your product:

<http://www.keysight.com/find/esa>

<http://www.keysight.com/find/emc>

To receive the latest updates by email, subscribe to Keysight Email Updates at the following URL:

<http://www.keysight.com/find/MyKeysight>

Information on preventing analyzer damage can be found at:

[www.keysight.com/find/PreventingInstrumentRepair](http://www.keysight.com/find/PreventingInstrumentRepair)

## Is your product software up-to-date?

Periodically, Keysight releases software updates to fix known defects and incorporate product enhancements. To search for software updates for your product, go to the Keysight Technical Support website at:

<http://www.keysight.com/find/techsupport>



<b>1. Preparing for Use</b>	
Description .....	8
Panel Description .....	8
Initial Inspection .....	9
Power Cable .....	9
<b>2. Installation and Operation</b>	
Battery Charging Procedure .....	14
Installing the Battery Pack .....	16
Installation Procedure .....	16
Operation .....	18
Basic Operation Check .....	18
<b>3. Characteristics</b>	
Characteristics .....	20
Typical Runtime .....	20
Regulatory Information .....	23
<b>4. Troubleshooting</b>	
Troubleshooting .....	26
Basic Troubleshooting .....	26
Troubleshooting the Battery Pack and the 24 VDC Charger Power Supply .....	26
Cleaning .....	29
Replacement .....	29
<b>5. Disposal and Service</b>	
Disposal .....	32
Battery Disposal .....	32
Contacting Agilent Technologies .....	33
Battery Pack Serial Numbers .....	33
Calling Agilent Sales and Service Offices .....	33
How to Order Parts .....	34
Direct Phone-Order System .....	34



---

# **1** **Preparing for Use**

This chapter describes the battery pack and provides initial inspection information.

---

## Description

The Agilent Technologies E1779A is a battery pack that will typically power an Agilent ESA Spectrum Analyzer or EMC Analyzer from 60 to 90 minutes, depending on the model number and the options installed in the analyzer. (See [Chapter 3, “Characteristics”](#) for more information about run time.)

## Panel Description


The battery pack has gold plated electrical contacts (1). A protective rubber safety boot (2) is attached to protect the contacts when the battery pack is not installed. A charging connector (5) is provided for attachment of the charger power supply. Adjacent to the charging connector are two LED indicator lights (4) to give visual information of the charging status. The latches (3) on each side of the battery pack are for attaching the battery pack to the analyzer. There is a hole (6) provided for the rubber safety boot plug to hold the boot in place when the battery pack is attached to the analyzer.

---

### CAUTION

The battery pack is *NOT* water resistant. It must be protected from liquids and other contaminants which could be spilled on the connector face.

**Figure 1-1**      **Battery Pack Description**

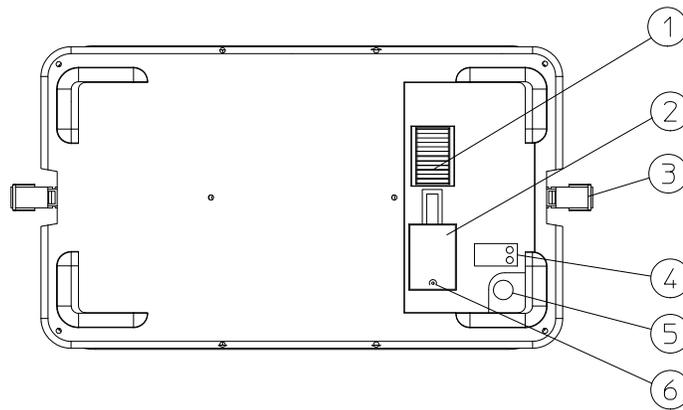


dv81a

## Initial Inspection

You should receive the following:

**Figure 1-2 E1779A Battery Pack Components**

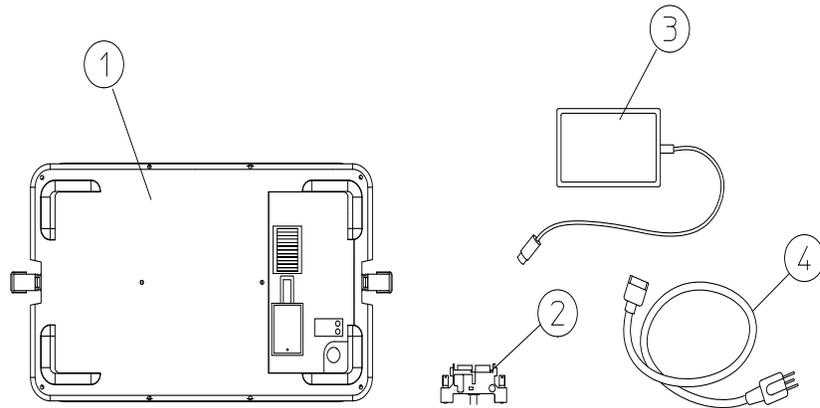

dv82a

Number	Description	Part Number
1	Battery Pack	None
2	DC Adapter	E4401-60025
3	Charger Power Supply	U2931-60012
4	AC Line Cord	See <a href="#">Figure 1-3 on page 11</a> .
	User's Guide	E1779-90015
	20 A Fuse Kit	E4401-60286

### Power Cable

The battery pack charger power supply is equipped with a three-wire power cable, in accordance with international safety standards. When connected to an appropriate power line outlet, this cable grounds the charger power supply case.

#### WARNING

**Failure to ground the charger power supply properly can result in personal injury. Insert the main power cable plug only into a socket outlet that has a protective earth contact. DO NOT defeat the earth-grounding protection by using an extension cable, power cable, or autotransformer without a protective ground conductor.**

**If you are using an autotransformer, make sure its common terminal is connected to the protective earth contact of the power source outlet socket.**

Various power cables are available to connect the charger power supply to the types of AC power outlets unique to specific geographic areas. You will receive the cable appropriate for the area to which the charger power supply is originally shipped. You can order additional AC power cables for use in different areas. The following table lists the available AC power cables, illustrates the plug configurations, and identifies the geographic area in which each cable is appropriate.

---

**CAUTION**

The battery pack should be removed when the analyzer is not being used, especially during transportation. The battery will continue to drain at a slow rate while attached to the analyzer. Over an extended period of time, the battery could discharge to the point that it irreversibly damages some of its nickel-cadmium cells, preventing the battery from being fully recharged.

---

Figure 1-3 Power Cables

Plug Type <sup>a</sup>	Cable Part Number	Plug <sup>b</sup> Description	Length cm (in.)	Cable Color	For Use in Country
250V 	8120-1351	Straight BS 1363A	229 (90)	Mint Gray	Option 900 United Kingdom, Hong Kong, Cyprus, Nigeria, Singapore, Zimbabwe
	8120-1703	90°	229 (90)	Mint Gray	
250V 	8120-1369	Straight AS 3112	210 (79)	Gray	Option 901 Argentina, Australia, New Zealand, Mainland China
	8120-0696	90°	200 (78)	Gray	
125V 	8120-1378	Straight NEMA 5-15P	203 (80)	Jade Gray	Option 903 United States, Canada, Brazil, Colombia, Mexico, Philippines, Saudi Arabia, Taiwan
	8120-1521	90°	203 (80)	Jade Gray	
125V 	8120-4753	Straight NEMA 5-15P	229 (90)	Gray	Option 918 Japan
	8120-4754	90°	229 (90)	Gray	
250V 	8120-1689	Straight CEE 7/VII	200 (78)	Mint Gray	Option 902 Continental Europe, Central African Republic, United Arab Republic
	8120-1692	90°	200 (78)	Mint Gray	
230V 	8120-2104	Straight SEV Type 12	200 (78)	Gray	Option 906 Switzerland
	8120-2296	90°	200 (78)	Gray	
220V 	8120-2956	Straight SR 107-2-D	200 (78)	Gray	Option 912 Denmark
	8120-2957	90°	200 (78)	Gray	
250V 	8120-4211	Straight IEC 83-B1	200 (78)	Mint Gray	Option 917 South Africa, India
	8120-4600	90°	200 (78)	Mint Gray	
250V 	8120-5182	Straight SI 32	200 (78)	Jade Gray	Option 919 Israel
	8120-5181	90°	200 (78)	Jade Gray	

a. E = earth ground, L = line, and N = neutral.

b. Plug identifier numbers describe the plug only. The HP part number is for the complete cable assembly.

plugs



---

## **2** **Installation and Operation**

This chapter provides the information needed to charge, install, and operate the Agilent E1779A battery pack.

## Battery Charging Procedure

---

### WARNING

**This is a Safety Class 1 Product when the battery is being charged and is provided with a protective earthing ground incorporated in the power cord. The mains plug shall only be inserted in a socket outlet provided with a protective earth contact. Any interruption of the protective conductor inside or outside of the product is likely to make the product dangerous. Intentional interruption is prohibited.**

---

### CAUTION

This product is designed for use in Installation Category II and Pollution Degree 2 per IEC 1010 and 664 respectively when being charged with the approved AC to DC supply.

Connect the AC line to the charger power supply so that the detachable power cord is readily identifiable and is easily reached by the operator. The detachable power cord is the disconnection device. It disconnects the charger power supply from the AC line. Alternatively, an externally installed switch or circuit breaker (which is readily identifiable and is easily reached by the operator) may be used as a disconnecting device.

Refer to [Figure 2-1](#).

1. Remove the battery pack (1) from the instrument.
2. Plug the charger power supply (2) into the battery pack.
3. Connect the AC line cord (3) to the charger power supply and to the AC line.

When the battery pack begins its charging cycle the red LED (5) will start flashing. The red LED will then become a solid red light. When the battery pack is fully charged, the green LED (4) will be lit.

---

### NOTE

Both LEDs will be lit if the internal temperature of the battery pack is above 55°C or below 10°C.

Continuing to charge the battery pack after the green LED is lit will not damage the unit. It will continue to charge in the trickle charge mode.

---

### CAUTION

Do not use any charger power supply other than that supplied with the battery pack.

---


### NOTE

At room temperature, it takes 6 hours to initially charge a battery, or charge a battery after it has been depleted on an analyzer while in use (battery voltage drained to ~15 VDC). Charging a fully depleted battery will take longer, possibly as long as 8 to 12 hours. Charging the battery at elevated temperatures will increase the charge time. Occasionally the battery should be fully discharged, to the depleted state, prior to charging. This will prevent degradation of battery capacity due to the memory effects exhibited by nickel-cadmium batteries.

---

Figure 2-1

Charging the Battery

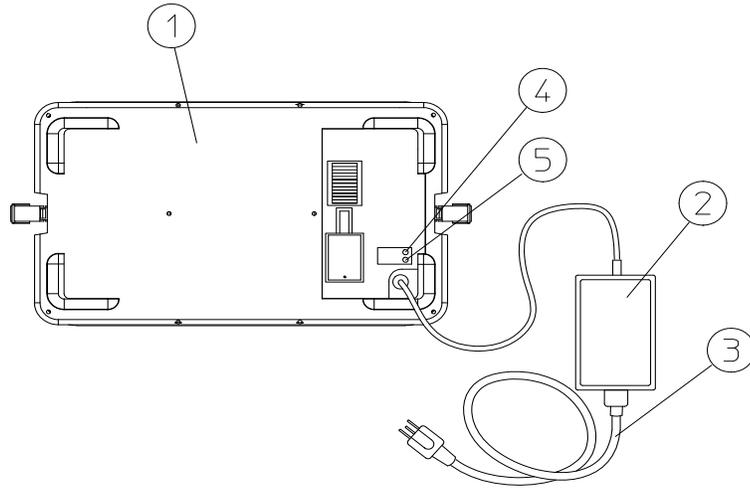

dv86a

## Installing the Battery Pack


- 
- WARNING** This battery pack cannot be plugged into Agilent E4411A analyzers with a serial number of US3736xxxx or below. The mating screws are keyed to ensure that this is not possible. Overriding the keyed safety feature could be dangerous.
- 
- NOTE** Analyzers with a serial number of US3736xxxx or below require the installation of Option R12 before the battery pack will operate.
- 
- NOTE** Remove the analyzer AC connector (power cord) prior to installing the battery.
- 
- CAUTION** Ventilation Requirements: When installing the product in a cabinet, the convection into and out of the product must not be restricted. The ambient temperature (outside the cabinet) must be less than the maximum operating temperature of the product by 4°C for every 100 watts dissipated in the cabinet.
- There is no need to make a wire connection when installing the battery pack. The DC contacts on the battery pack press against the contacts of a DC adapter which plugs into the 12 VDC input connector on the analyzer. The battery pack is installed by attaching the latches on each side of the battery pack to the analyzer.
- Install the product according to the enclosure protection code IP 32. There is protection against the entrance of solid foreign objects that are greater than 2.5 mm in diameter and water that is dripping at an angle of less than 15 degrees.
- 
- NOTE** The DC connector system is designed to ensure very little power loss so that all necessary power is supplied to the analyzer. Right angle connectors are required for rear panel connections when the battery pack is attached.
- 

## Installation Procedure

Use the following procedure to install the battery pack to your analyzer:

1. Remove the power cord from the analyzer.
2. Attach the DC adapter (2) to the rear panel of the analyzer. The adapter has no polarity. Tighten the two screws.
3. Uncover the battery DC contacts by securing the safety boot in its open position.
4. Attach the battery pack (3) to the back of the analyzer. Battery pack contacts should align with the DC adapter.
5. Fasten the latches (4) on each side of the battery pack to the analyzer. Turn the analyzer on and begin DC operation.

Figure 2-2 Battery Pack Installation

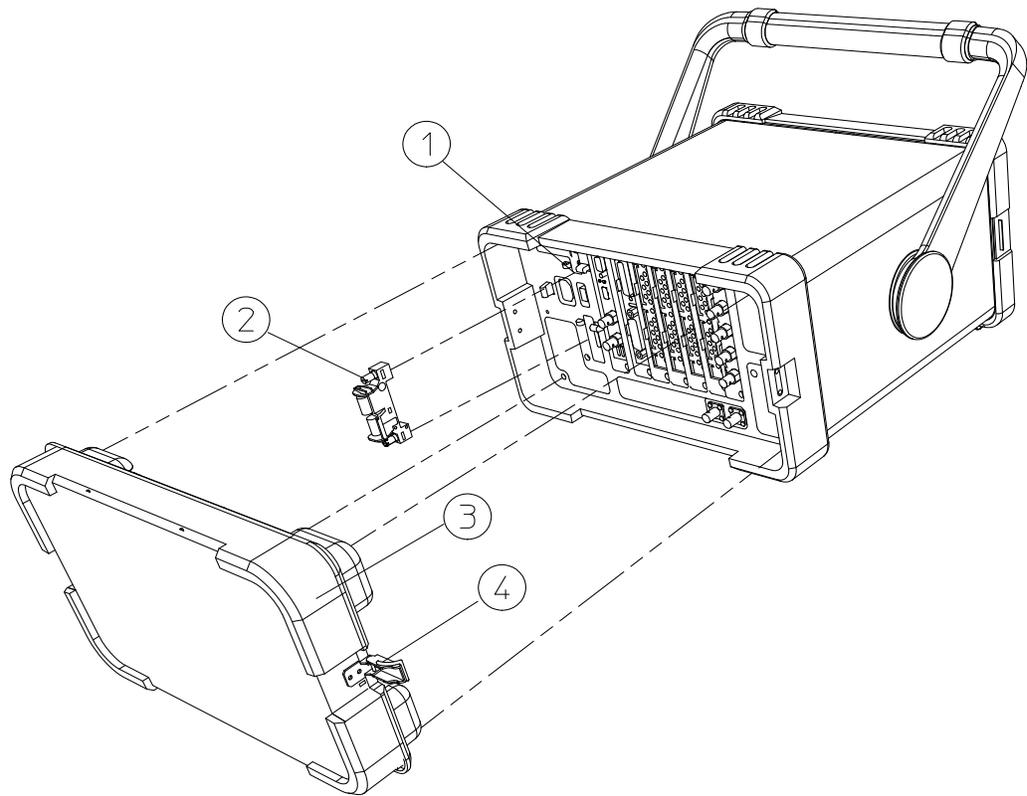

dv85a

## Operation

---

**WARNING** Shorting the battery pack contacts will result in unrepairable damage to the contacts and internal circuit. There is also the danger of burns. Use the safety boot to cover the contacts any time the battery pack is removed from the instrument.

---

**WARNING** The power cord must not be installed with the battery pack in place.

---

**WARNING** The charger power supply must not be connected to the battery pack when the battery pack is attached to the analyzer.

---

An Agilent ESA Spectrum Analyzer or EMC Analyzer will operate with the same functionality on DC power as it will on AC power except that the line trigger will not function.

### Basic Operation Check

The only basic operation checks for the battery pack are whether or not it takes a charge, and whether or not the instrument powers on when the battery pack is installed.

The battery pack has no operational specifications and is therefore not subject to periodic calibration.

---

**WARNING** No serviceable parts inside. Do not disassemble.

---

---

## **3** **Characteristics**

This chapter contains information about the characteristic operating parameters of the Agilent E1779A battery source. Characteristics provide useful but non-warranted information about the functions and performance of the battery pack.

---

## Characteristics

---

**NOTE** All characteristics are at 25 °C and at the beginning of battery life.

<b>Output Voltage</b>	19.2 volts
<b>Capacity</b>	105 watt hours
<b>Service Life</b>	500 Cycles to 80% Initial Capacity (at 25°C)

### Typical Runtime

Runtime is typically between 60 minutes and 90 minutes depending upon options installed.

<b>Chemistry</b>	Nickel-Cadmium
<b>Charge Time</b>	6 Hours <sup>a</sup>
<b>Charging Temperature</b>	10°C to 40°C <sup>b</sup>
<b>Discharging Temperature</b>	0°C to 55°C <sup>b</sup>
<b>Storage Temperature</b>	-30°C to 55°C <sup>b</sup>
<b>Maximum Relative Humidity</b>	80% <sup>c</sup>

- Charge time may exceed 6 hours at temperatures above 25°C.
- Refer to the following graphs for temperature impact on battery performance and service life.
- For temperatures up to 31°C. Maximum relative humidity will decrease linearly to 50% at 40°C.


---

**CAUTION** Battery service life degrades rapidly at temperatures above 40°C. This effect can be minimized if it is held for only a short period of time at the high temperature, such as during discharge. Prolonged storage at only 40°C could reduce the service life to 45% of its room temperature life. The service life is reduced to 20% at 50°C.

---

Figure 3-1


Battery Charge Capacity vs Temperature

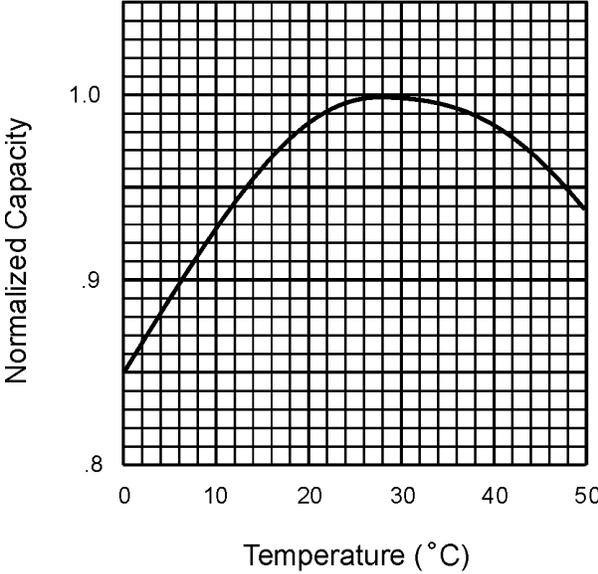

dv87a

Figure 3-2


Battery Cycle Life vs Temperature

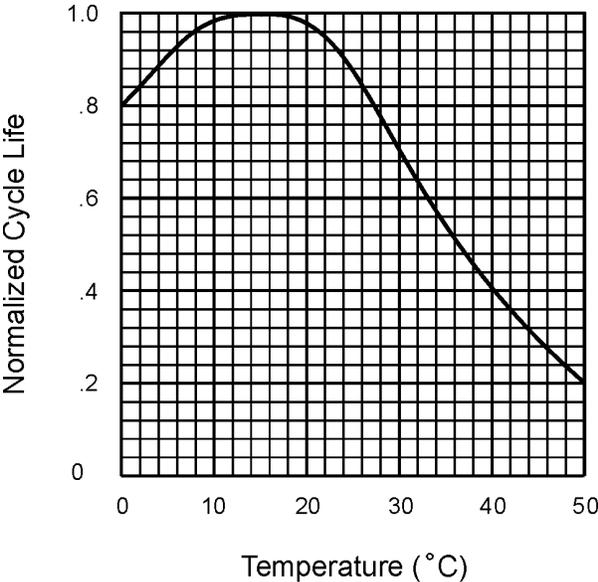

dv88a

**Figure 3-3**

**Battery Charge Acceptance versus Temperature**

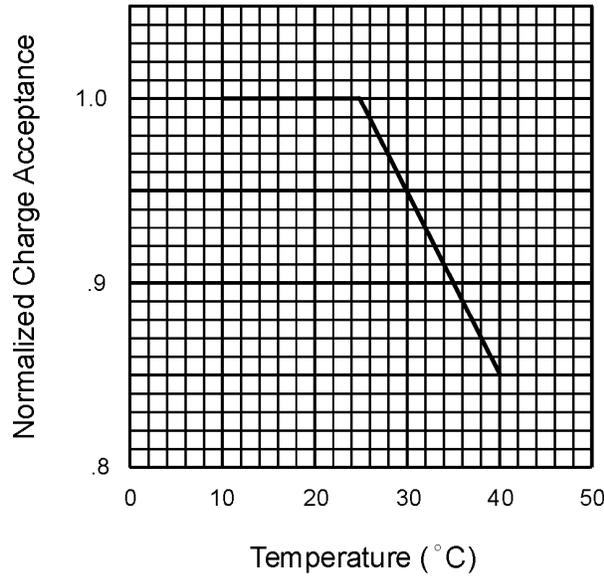

dv89a

<b>Physical Characteristics</b>	
Weight	4.8-kg (10.6-lbs)
Height	217-mm (8.54-in)
Width	373-mm (14.69-in)
Depth	68-mm (2.68-in), 44-mm (1.73-in) added to instrument depth

<b>Supply Requirements</b>	
Nominal Input Voltage	100/115/230/240 Volts
Input Voltage Range	90-254 Volts
Nominal Input Frequency	50/60 Hz
Input Frequency Range	47-66 Hz
Input Power	60 Watts Maximum
Output Voltage	24 VDC

<b>Environmental Conditions</b>
Portable
Altitude up to 4,572 meters (15,000 feet)
This product, when being recharged with the approved ac to DC supply, is designed for use in INSTALLATION CATEGORY II and POLLUTION DEGREE 2, per IEC 1010 and 664 respectively.

---

## Regulatory Information

---

### CAUTION

This product is designed for use in Installation Category II and Pollution Degree 2 per IEC 1010 and 664 respectively.

---

### NOTE

This product has been designed and tested in accordance with IEC Publication 1010, Safety Requirements for Electronic Measuring Apparatus, and has been supplied in a safe condition. The instruction documentation contains information and warnings which must be followed by the user to ensure safe operation and to maintain the product in a safe condition.




The CE mark is a registered trademark of the European Community.



The CSA mark is the Canadian Standards Association safety mark.

ISM 1-A

This is a symbol of an Industrial Scientific and Medical Group 1 Class A product. (CISPR Pub. 11, Clause 4)



This is a symbol to alert you that you must dispose of a material properly according to your country's requirements and not just throw it into the trash.

## DECLARATION OF CONFORMITY

According to ISO/IEC Guide 22 and CEN/CENELEC EN 45014

**Manufacturer's Name:** Agilent Technologies, Inc.

**Manufacturer's Address:** 1400 Fountaingrove Parkway  
Santa Rosa, CA 95403-1799  
USA

Declares that the product

**Product Name:** Battery Pack

**Model Number:** E1779A

**Product Options:** This declaration covers all options of the above product.

Conforms to the following product specifications:

EMC: IEC 61326-1:1997+A1:1998 / EN 61326-1:1997+A1:1998

<u>Standard</u>	<u>Limit</u>
CISPR 11:1990 / EN 55011-1991	Group 1, Class A
IEC 61000-4-2:1995+A1998 / EN 61000-4-2:1995	4 kV CD, 8 kV AD
IEC 61000-4-3:1995 / EN 61000-4-3:1995	3 V/m, 80 - 1000 MHz
IEC 61000-4-4:1995 / EN 61000-4-4:1995	0.5 kV sig., 1 kV power
IEC 61000-4-5:1995 / EN 61000-4-5:1996	0.5 kV L-L, 1 kV L-G
IEC 61000-4-6:1996 / EN 61000-4-6:1998	3 V, 0.15 - 80 MHz
IEC 61000-4-11:1994 / EN 61000-4-11:1998	1 cycle, 100%

Safety: IEC 61010-1:1990 + A1:1992 + A2:1995 / EN 61010-1:1993 +A2:1995  
CAN/CSA-C22.2 No. 1010.1-92

**Supplementary Information:**

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC and carries the CE-marking accordingly.

This product was tested with Agilent Technologies ESA Series Spectrum Analyzers.



Santa Rosa, CA, USA 7 Oct. 2000

Greg Pfeiffer/Quality Engineering Manager

For further information, please contact your local Agilent Technologies sales office, agent or distributor.

---

## **4 Troubleshooting**

This chapter provides information on how to troubleshoot your battery pack.

## Troubleshooting

Your battery pack is built to provide dependable service during the service life of the ni-cad batteries. However, if you experience a problem, desire additional information, or wish to order parts, Agilent's worldwide sales and service organization is ready to provide the support you need.

### Basic Troubleshooting

If the battery pack does not work, follow these steps to determine the cause and resolve the problem:

1. Make sure the analyzer works with ac power. If it does not, follow the troubleshooting procedures in the analyzer user's guide.
2. If the analyzer operates on ac power, but not on DC power:
  - a. Check all of your connections. Is the DC adapter firmly in place? Are the battery contacts aligned with the DC adapter?
  - b. Check the 20 A 32 VDC fuse on the analyzer. Replace it if it is blown. (Refer to [Figure 4-2 on page 28.](#))
3. Make sure that the battery pack is taking a charge from the charger power supply. Follow the recharging procedure. Usually batteries near the end of their life will still take a partial charge. If there is no charge at all, you may need to replace the charger power supply or the battery pack.

If you are not sure whether the cause of failure is the battery pack or the charger power supply, follow the troubleshooting procedures below, or send your battery pack and charger power supply to a service center for diagnosis. Sending both the battery pack and the charger power supply will ensure a complete analysis.


### Troubleshooting the Battery Pack and the 24 VDC Charger Power Supply

Follow these steps to determine whether the battery pack or the charger power supply is defective:

1. Check the charger power supply for 24 VDC  $\pm 10\%$  by measuring its voltage under load with an autoranging multimeter.

Refer to [Figure 4-1](#) when performing the following steps:

**Figure 4-1**      **Charger Supply Load Test Fixture**

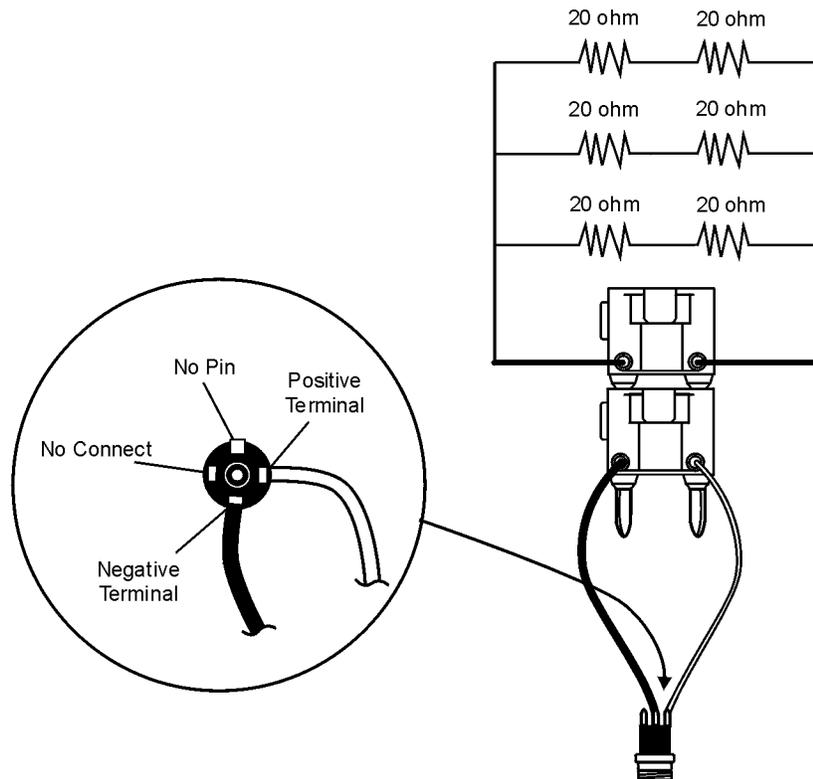

dv11a

- a. Strip the ends of two four-inch pieces of 16 AWG wire, one white and one black.
- b. Solder one end of the black wire to the negative terminal (center solder lug) of a 2.5 mm male barrel jack (part number 1252-5866), and one end of the white wire to the positive terminal (refer to [Figure 4-1](#)). Leave the third terminal of the male barrel connector unconnected.
- c. Plug the two wires from the barrel jack into the terminals of a dual banana plug (part number 1251-0005) and plug this into the multimeter.
- d. Solder together 3 pairs of 20  $\Omega$  20 W resistors (part number 0811-1656) in parallel to create the 13.3  $\Omega$  120 W equivalent circuit shown in [Figure 4-1](#).
- e. Connect this 13.3  $\Omega$  circuit to the lead terminals of a second dual banana plug and plug this into the first dual banana plug.
- f. Plug the charger power supply's barrel plug into the barrel jack.
  - If a voltage of 24 VDC  $\pm$ 10% is not present, it indicates that the charger power supply is defective. Avoid leaving the charger power supply connected for more than 1 or 2 minutes since the resistors get very hot.

---

**WARNING**

**The resistors will get very hot. Handle with care.**

2. If the correct charger power supply voltage (24 VDC  $\pm$ 10 %) is present, plug the charger power supply into the battery pack and ensure that the red LED flashes, then remains on.

---

**NOTE**

The red LED should turn on and the battery should charge initially even if the battery pack is fully

charged.

If the green LED turns on immediately, this indicates a defective battery pack. If the red LED continues blinking, this indicates that the battery pack voltage is below 16 VDC. The battery will charge in trickle mode until this condition no longer exists. If this condition continues longer than 24 hours, this also indicates a defective battery pack.

3. If the red LED flashed and then remained on, as expected, confirm that the battery charges correctly by probing the battery pack contacts with the multimeter. The charger power supply will start charging the battery initially even if the battery is fully charged. The voltage should gradually increase, indicating that the battery is charging. If the voltage does not increase by several hundredths of a volt over a period of 1 to 2 minutes, this indicates that the battery is not charging properly. You may wish to retry the test by unplugging and then plugging in the charger power supply again. If the battery still does not charge, unplug the charger power supply and replace it with a known good charger power supply and repeat the test. If the battery charges, this indicates that the original charger power supply is defective. If the battery does not charge with a new charger power supply, this indicates that the battery pack is defective.

**NOTE**

Both LEDs will be lit if the internal temperature of the battery pack is above 55°C or below 10°C.


4. If all three of these tests pass, it indicates that the charger power supply and the battery pack are both working.

**NOTE**

Defective battery packs should be discarded according to individual country's requirements.

**Figure 4-2**

**DC Adapter Plug and Fuse**

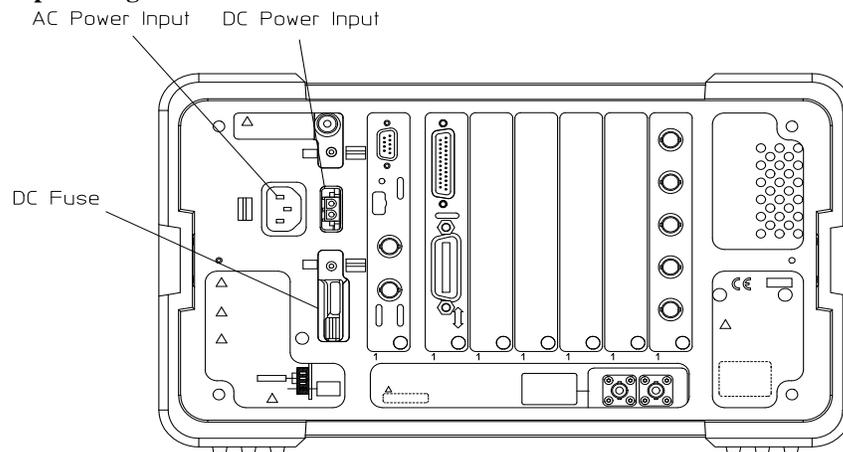

dv810a

**Cleaning**

The battery pack contacts will provide good service over the life of the assembly. Should they become contaminated, clean by wiping gently with a clean dry cloth.

**Replacement**

When run time is unacceptable, replace the battery pack. The battery pack cannot be opened for repair.

The only replaceable parts are the charger power supply, the DC adapter, the power cord, and the safety boot.

### Latch Replacement


If the latch (1) to the battery pack needs to be replaced, order part number 1390-1061. Remove the two screws (part number 0515-0433) holding the latch in place, and attach the new latch.

### Safety Boot Replacement

To replace the safety boot (2), order part number E4401-40022 from Agilent. Cut the remaining parts of the old safety boot from the battery pack. Insert the feet of the new safety boot into the holes provided.

Figure 4-3

### Replaceable Parts

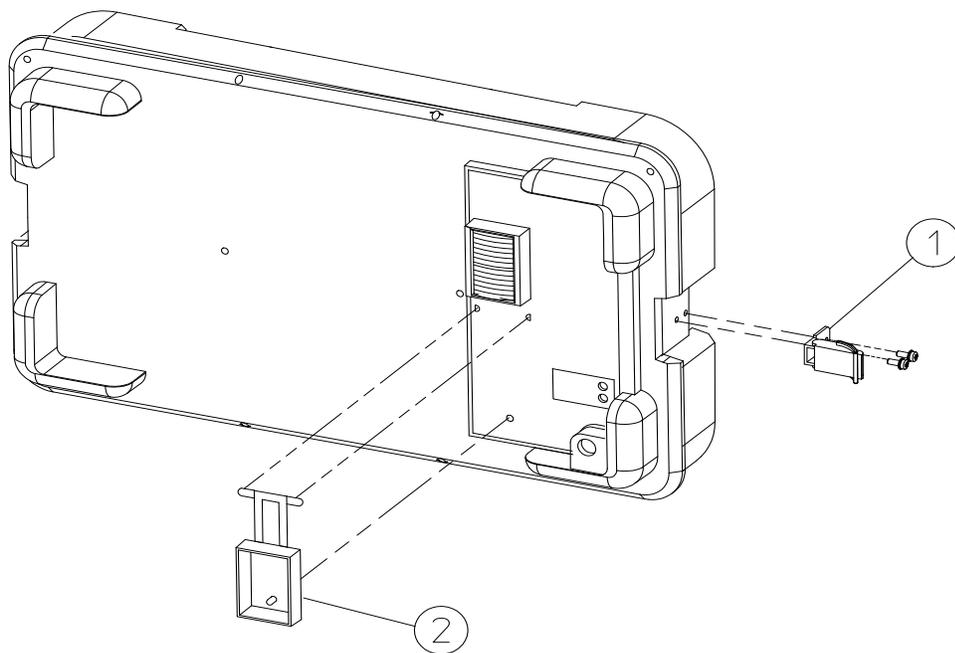

dv83a



---


## **5**      **Disposal and Service**

This chapter provides information on disposing of your battery pack when its service life is gone, and on contacting Agilent Technologies for service.

## **Disposal**

### **Battery Disposal**

When the batteries are exhausted and/or ready for disposal, dispose of them according to your country's requirements.

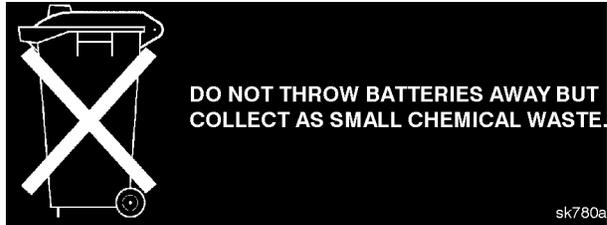

---

## Contacting Agilent Technologies

If you have a problem with your battery pack, check the troubleshooting steps earlier in [Chapter 4](#), “[Troubleshooting](#),” or return the battery pack to Agilent.

### Battery Pack Serial Numbers

Agilent makes frequent improvements to its products to enhance performance, usability, or reliability. Our service personnel have access to complete records of design changes to each type of product, based on the serial number and option designation.

Whenever you contact Agilent Technologies about your battery pack, have the complete serial number available. This will ensure that you obtain accurate service information.

The serial number label is attached near the DC output connector on the battery pack.

The serial number has two parts: the prefix (two letters and the first four numbers), and the suffix (the last four numbers). Refer to [Figure 5-1](#).

**Figure 5-1**

#### Example Serial Number



The two letters identify the country in which the battery pack was manufactured. The four numbers of the prefix are a code identifying the date of the last major design change incorporated into the battery pack. The four digit suffix is a sequential number, and coupled with the prefix, provides a unique identification for each battery pack produced. Whenever you list the serial number or refer to it in obtaining information about the battery pack, be sure to use the complete number, including the full prefix and suffix.

### Calling Agilent Sales and Service Offices

Agilent’s sales and service offices are located around the world to provide complete support for your battery pack. To obtain servicing information or to order replacement parts, contact the nearest Agilent Sales and Service office listed in [Table 5-1](#). In any correspondence or telephone conversations, refer to the battery pack by its model number and full serial number. With this information, the representative can quickly determine whether your battery pack is still within its warranty period.

### How to Order Parts

To order an assembly or part, quote the Agilent part number and indicate the quantity required.

If you do not have the part number, include the following information with the order:

- Model number
- Serial number
- Description of where the part is located, what it looks like, and its function (if known).
- Quantity

Parts can be ordered by addressing the order to the nearest Agilent office. Customers within the USA can also use either the direct mail-order system, or the direct phone-order system described below. The direct phone-order system has a toll-free phone number available.

### **Direct Phone-Order System**

Within the USA, Agilent can supply parts through a direct mail-order system. Advantages of using the system are as follows:

- Direct ordering and shipment from Agilent.
- No maximum or minimum on any mail order. (There is a minimum order amount for parts ordered through a local office when the orders require billing and invoicing.)
- Prepaid transportation. (There is a small handling charge for each order.)
- No invoices.

To provide these advantages, a check or money order must accompany each order. Mail-order forms and specific ordering information are available through your local Agilent office.

By internet, phone, or fax, get assistance with all your test and measurement needs.

**Table 5-1 Agilent Sales and Services Offices**

**Online assistance:** [www.agilent.com/find/assist](http://www.agilent.com/find/assist)

<p><b>United States</b> (tel) 1 800 452 4844</p>	<p><b>Japan</b> (tel) (+81) 426 56 7832 (fax) (+81) 426 56 7840</p>	<p><b>New Zealand</b> (tel) 0 800 738 378 (fax) (+64) 4 495 8950</p>	<p><b>Europe</b> (tel) (+31) 20 547 2323 (fax) (+31) 20 547 2390</p>
<p><b>Canada</b> (tel) 1 877 894 4414 (fax) (905) 282 6495</p>	<p><b>Latin America</b> (tel) (305) 269 7500 (fax) (305) 269 7599</p>	<p><b>Australia</b> (tel) 1 800 629 485 (fax) (+61) 3 9210 5947</p>	

**Asia Call Center Numbers**

Country	Phone Number	Fax Number
Singapore	1-800-375-8100	(65) 836-0252
Malaysia	1-800-828-848	1-800-801664
Philippines	(632) 8426802 1-800-16510170 (PLDT Subscriber Only)	(632) 8426809 1-800-16510288 (PLDT Subscriber Only)
Thailand	(088) 226-008 (outside Bangkok) (662) 661-3999 (within Bangkok)	(66) 1-661-3714
Hong Kong	800-930-871	(852) 2506 9233
Taiwan	0800-047-866	(886) 2 25456723
People's Republic of China	800-810-0189 (preferred) 10800-650-0021	10800-650-0121
India	1-600-11-2929	000-800-650-1101

